



THE MINI-300 SERIES

Operating and Service Manual

Series includes all variants of MINI-300/310

Issue B
September 2015



TABLE OF CONTENTS

1. Description	3
2. Installation	3
3. Operation	4
4. Special Conditions for Safe Use	4
5. Hazardous Location Usage	4
6. Servicing and Maintenance.....	4
6.1. Servicing the MINI-300 (LP)	5
6.1.1. Accessing the Main Valve Assembly	5
6.1.2. Adjusting the Set Point	6
6.1.3. Figure 1 – Sectional View of the MINI-300 (LP)	7
7. Technical Data.....	8
8. Warranty Statement	8
Annex A. The 310 – ‘Solid Disk’ Main Valve Design	9
A.1. Description.....	9
A.2. Servicing.....	9
A.2.1. Figure 2 – Detail A: The 310 ‘Solid Disk’ MVA (sectional)	9
A.2.2. Figure 3 – Exploded View of the 310 ‘Solid Disk’ MVA	9

1. Description

MINI-300 is a 'compact' single stage piston sensed pressure regulator, capable of a maximum 210bar inlet pressure (300bar with PEEK seat). The standard units utilise two piston sensing options, a 20mm 'Low Pressure' sensor and also an 8mm 'High Pressure' sensor. The Low Pressure (LP) option will control the outlet pressure up to a maximum of 10bar. The High Pressure (HP) option allows control of the outlet pressure up to a maximum of 100 bar. A modification is also available allowing the MINI-300-HP option to achieve up to 210 bar outlet pressure.

The housing has been machined from all 316 stainless steel to ensure maximum protection against the media on which it will be used, and the environment in which it will be placed.

2. Installation

Before system start-up, it is recommended that all systems be pressure tested, leak tested and purged with an inert gas such as nitrogen.

Prior to placing into service ensure that the regulator is in the fully closed position, with the adjusting mechanism turned completely anti-clockwise.

Check the model number reference to ensure that the pressure range complies with the installation requirements.

Visually inspect the regulator for any signs of damage or contamination. If any foreign materials are present and cannot be removed from the regulator, or if the threads on the regulator appear to be damaged, please contact the office immediately to arrange for the regulator to be returned for service.

The Inlet and Outlet ports are clearly marked. Select the correct size and type of connection fittings for these ports which are indicated in the regulators part number. Both British Standard Pipe (BSPP) 'B' and National Pipe Thread (NPT) 'N' options are available on this regulator. Use the correct dowty or bonded seal for BSPP connections, self centering seals are recommended. For NPT threads, ensure that PTFE tape is applied correctly to the fittings, applying two overlapping layers in the direction of the thread, taking care that the tape does not come into contact with the first thread.

Any gauge ports on the regulator will be 1/8" NPT unless otherwise stated. If any gauge port is not required, ensure that the port is plugged prior to installation.

The media supplied to the regulator must be clean. Contamination can damage the seat which may cause the regulator to fail. Filtration suited to the application is recommended upstream of the regulator.

Should further assistance or information be required in relation to installation of any Pressure Tech regulator please contact the office, giving reference to the regulators part number and/or serial number.

3. Operation

Turning the adjusting mechanism clockwise compresses the spring, which in turn opens the main valve and allows the inlet pressure to pass through the seat orifice until the outlet pressure is equivalent to the loading forces set by the compressed spring. Increase the outlet pressure in this way until the desired pressure is achieved.

To reduce the outlet pressure, the adjusting mechanism should be turned anti-clockwise whilst the media is flowing, or whilst venting downstream of the regulator.

The desired outlet pressure should be set whilst increasing the pressure. Do not exceed the maximum inlet and outlet pressures of the regulator which are indicated on the regulator label.

4. Special Conditions for Safe Use

The MINI-300 series are non-venting type regulators, therefore the outlet pressure shall be reduced by venting downstream of the regulator whilst simultaneously turning the adjusting mechanism anti-clockwise.

5. Hazardous Location Usage

This equipment has not been manufactured specifically for use in potentially explosive atmospheres and as such an ignition hazard assessment has not been carried out on this product. If the user should wish to use this product in such an environment where there may be a potentially explosive atmosphere then it is the responsibility of the user to conduct an ignition hazard assessment against 99/92/EC.

6. Servicing and Maintenance

Servicing and maintenance work on the MINI-300 regulators should only be performed after fully reading and understanding the Operating and Servicing Manual. Due to the typical nature of the gases the regulator can be used with, the operator should not endanger himself/herself or others by working on this regulator without prior knowledge on the Health and Safety concerns relating to handling of technical gases. Any uncertainty should be clarified with Pressure Tech before working on the regulator.

Pressure Tech Ltd recommends the use of Krytox GPL 205 during servicing.

Prior to commencing service, please ensure that:

- The equipment has been de-pressurised
- The load spring has been de-compressed by turning the adjusting mechanism fully anti-clockwise
- Applications involving toxic, flammable or corrosive media have been fully purged

To ensure the best possible results from servicing, when re-assembling the regulator and any assemblies within it, ensure that all areas of the components and the regulator body are cleaned and free from contaminants which may result in failure of the regulator.

6.1. Servicing the MINI-300 (LP)

*Note: fig 1 should be used as a reference for the following set of instructions

6.1.1. Accessing the Main Valve Assembly

To access the Main Valve Assembly (MVA):

- i. With the flats of the Regulator Body (1) secured in a vice, loosen the Bonnet (12) using a 28mm wrench ensuring that the Hand Wheel (19) is fully wound anti clock wise (**Ref. 6.1.2*)
- ii. Remove the Upper LP Spring Rest (10), 6mm Ball Bearing (9), Load Spring (11), Sensor (8) from the assembly
- iii. The Seat Nut (7) can then be removed using a 12mm socket
- iv. Remove the Main Valve (4, 5) and Main Valve Spring (6) from the assembly
- v. Visually inspect the seat nut and soft seat (5) for damage under a microscope
- vi. Replace the Main Valve Spring (6) and Main Valve (4, 5) and place into the Regulator Body (1)
- vii. Replace Seat Nut (7) fitted with new 5x1 mm O-ring (17) taking care not to damage its sealing face against the tip of the valve
- viii. Replace the BS 020 O-ring (18) on the Sensor (8) and position into the regulator body (1)
- ix. Place the Load Spring (11), Upper LP Spring Rest (10) and 6mm Ball Bearing (9) on to the sensor (8)
- x. Screw the Bonnet (12) onto the assembly and using a torque wrench with a 28mm open ended attachment, tighten to 40Nm

It is recommended that all parts in the repair kits are used. Any defect parts removed during the service should be disposed of. Parts should be kept clean in line with media requirements. Following re-assembly of the regulator, pressure tests should be made to both the inlet and outlet side of the regulator, to ensure there is no internal or external leakage across the regulator.


To ensure that the main valve assembly has been correctly and effectively installed it may be required to perform the appropriate seat leak test as per ANSI/FCI 70-2.

6.1.2. Adjusting the Set Point

It is not recommended (or necessary) to remove the Hand Wheel during service as this will affect the set point of the regulator. Should it be required to adjust the set point please follow the instructions below:

- i. Remove the Nameplate (20) and Cap from the Hand Wheel (19) and loosen the Lock Nut (14) such that the Hand Wheel is able to spin freely on the Adjusting Screw (13)
- ii. Connect the correct fittings to the Inlet and Outlet ports of the regulator. Ensure that any gauge ports are plugged or that the correct gauge is fitted
- iii. With the Regulator Body (1) secured in a vice apply the Maximum Working Pressure (MWP) to the Inlet of the regulator
- iv. Connect the Outlet port to a calibrated pressure test gauge appropriate to the required set pressure. As the regulator is non-venting, ensure that a ball/needle valve is fitted to allow pressure to be relieved downstream of the regulator
- v. Using a slotted screwdriver, turn the Adjusting Screw (13) clockwise until the desired set point has been reached
- vi. Ensure repeatability by allowing flow through the regulator using the ball/needle valve
- vii. With the outlet pressure set, screw the first Lock Nut (14) to the base of the Adjusting Screw (13) against the Bonnet (12)
- viii. Position the Hand Wheel (19) onto the Lock Nut (14). Ensure that the Lock Nut and Hand Wheel become engaged
- ix. Fasten the second Lock Nut (14) against the Hand Wheel (19) and gently begin to tighten using a 13mm socket until it begins to secure itself
- x. At this point, whilst holding the Hand Wheel (19) continue to tighten whilst simultaneously turning slightly anti-clockwise to prevent it from locking against the Bonnet (12)
- xi. Ensure that the Lock Nut (14) is sufficiently tightened, taking care not to adjust the set point
- xii. Turning of the Hand Wheel (19) should now also turn the Adjusting Screw (13) which will control the pressure
- xiii. Turn the Hand Wheel clockwise until it reaches its set point and check to make sure that the desired outlet pressure is correct.
- xiv. If the set point is not correct, repeat steps v. to xiii.
- xv. Reduce the pressure downstream by venting the pressure through ball/needle valve and then turning the Hand Wheel anti-clockwise until the regulator closes
- xvi. The Cap and Nameplate (20) can now be placed into the Hand Wheel (19). Ensure that the information stated on the Nameplate (20) is in accordance with the set pressure of the regulator

6.1.3. Figure 1 – Sectional View of the MINI-300 (LP)

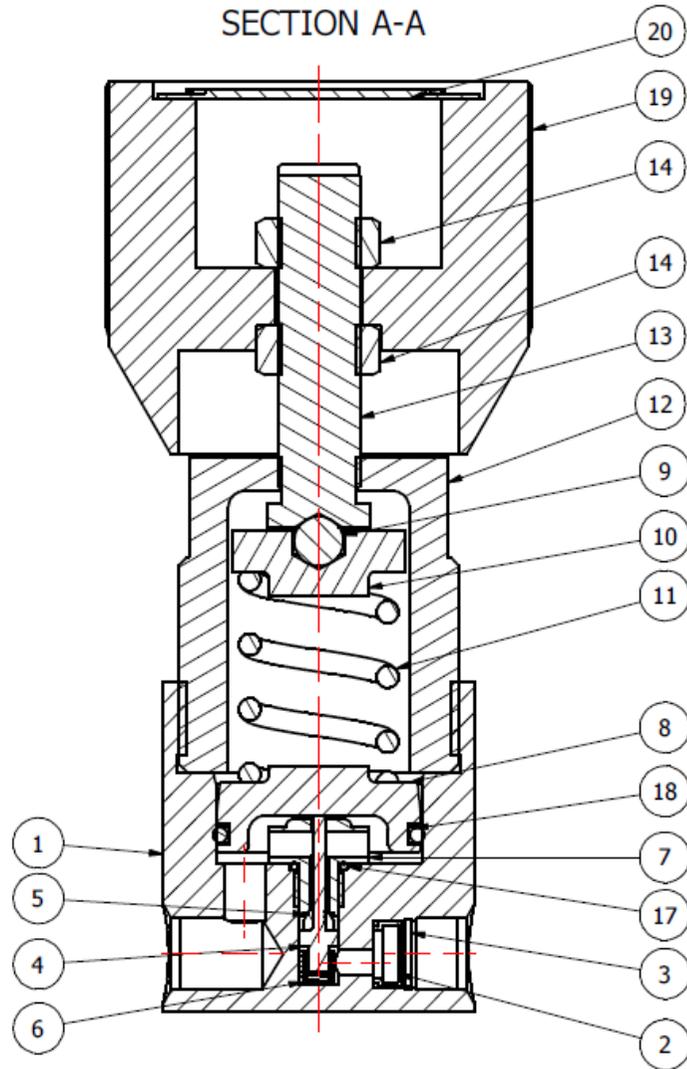

PARTS LIST		
ITEM	PART NUMBER	DESCRIPTION
1	PT-MINI-300-N-SS	1/8" NPT BODY
2	FILT-SCRM3803040S	8MM DIA SCREEN FILTER
3	CIRCLIP-DIN472-8MM	CIRCLIP
4	PT-C-001-013	MAIN VALVE WITH SQUARE
5	PT-C-002-011	PCTFE SEAT (210BAR)
6	PT-C-006-002	MAIN VALVE COMPRESSION SPRING
7	PT-C-007-002	SEAT Cv 0.06
8	PT-MINI-300-005	SENSOR 25MM
9	BALL-006-SS-316	6MM BALL BEARING
10	PT-MINI-300-003	SPRING REST LP
11	PT-C-011-009	LOAD SPRING
12	PT-MINI-300-004	BONNET
13	PT-C-019-003	ADJUSTING SCREW
14	PT-C-020	LOCKNUTS
17	OR-0050-10	O' RING STD
18	OR-BS020	O' RING STD
19	PT-C-021	SMALL HANDWHEEL
20	PT-C-022	NAMEPLATE

7. Technical Data

Fluid Media:	All gases and liquids compatible with materials of construction
Max Inlet Pressure*:	210 bar (3000 Psi) (with PCTFE Seat) 300 bar (4350 Psi) (with PEEK Seat)
Outlet Pressure Range:	0-10 bar (0-150 Psi) (Low Pressure MINI) 0-100 bar (0-1500 Psi)(High Pressure MINI) 0-210 bar (0-3000Psi) (Modified High Pressure MINI)
Operating Temperature:	-20°C to +80°C
Materials:	Body and Trim: 316 SS Seat: PCTFE / PEEK® / PTFE / FEP
Flow Capacity (Cv):	0.06 (also available in 0.03 and 0.15)
Leakage:	Gas: Bubble tight Liquid: Zero drops of water at max inlet

*Max Inlet Pressure determined by seat material and Cv of regulator.

8. Warranty Statement

Pressure Tech Ltd guarantee all products correspond with their specification at the time of delivery and, with exception to wear and tear, wilful damage, negligence, and abnormal working conditions, will be free from defects for a period of 12 months from date of delivery.

Annex A. The 310 – ‘Solid Disk’ Main Valve Design

A.1. Description


The ‘solid disk’ type main valve assembly was introduced as an alternative to the unique ‘cone type’ assembly and could be applied where greater resistance to both temperature and pressure were required. The new disk design allows for a wider range of seat material options as well as increased Cv and Pressure combinations.

The model number ‘310’ was assigned to denote the requirement for the new disk type main valve arrangement. The MINI-310 ‘solid disk’ option allows for a Maximum Working Pressure of 300 Bar (4350 Psi) or 414 bar (6000 Psi) when fitted with a PEEK seat. The MINI-310 is capable of controlling pressures of up to 100 bar (1500 Psi).

A.2. Servicing

The servicing of the MINI-310 regulator should be performed in line with the service instructions for the MINI-300 as defined in Section 6 of this manual, taking account for the difference in valve assembly. The figures below detail the alternate main valve assembly for reference purposes only.

A.2.1. Figure 2 – Detail A: The 310 ‘Solid Disk’ MVA (sectional)

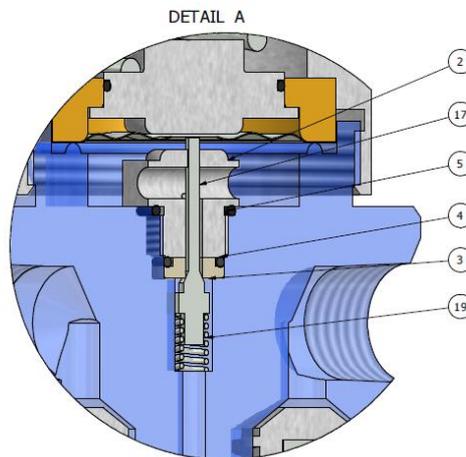

A.2.2. Figure 3 – Exploded View of the 310 ‘Solid Disk’ MVA

